RADIOLOGICAL IMAGING TECHNOLOGY, INC.

RIT113 Starshot Report

Analyzed Image


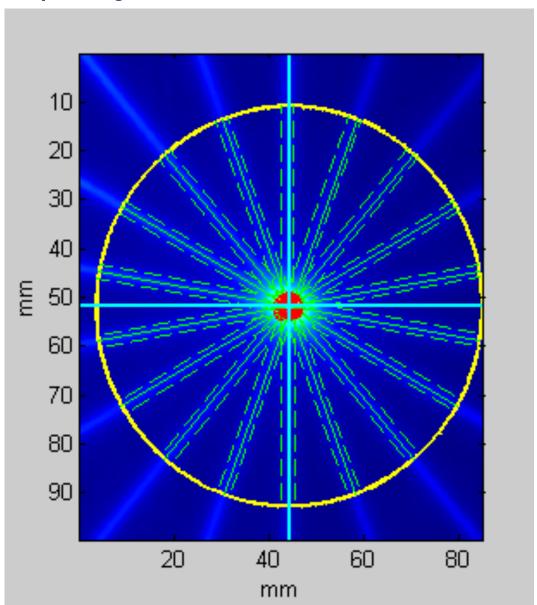


Image Information

Image File C:\RIT\RIT113V4\Demo Images\StarShot\fullstar.rv4

Detailed Plot

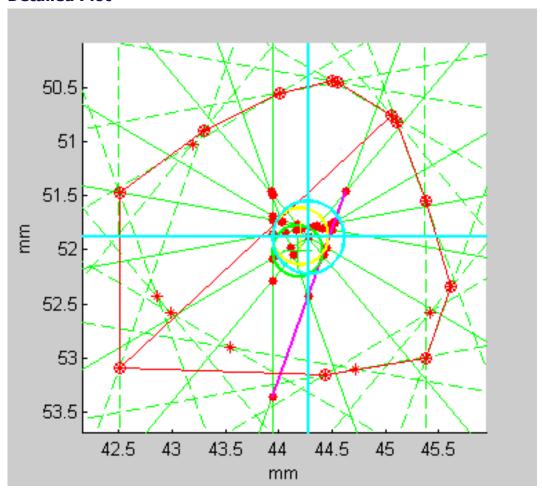

Analysis Results

Furthest Distance between Beam Center Intersections	2 mm
Maximum Distance across Beam Edge Intersections	3.5 mm
Mean Beam Width	2.7 mm
Minimum Tangent Circle Radius (TG142)	0.24 mm
Maximum Perpendicular Distance to Beam from Intersection Center	0.26 mm
Maximum Perpendicular Distance to Beam from User Defined Center	0.34 mm

Settings

Number of Legs (2 x # Beams)	18
Threshold	20%